SAFETOUCH™

Huber Infusion set

Securing the Huber Needle



The silicone coating offers smoother insertion and less effort for the patient during placement and removal.

Take care to follow these practical steps for a secure fixation and stabilization of the needle and tubing.

1. Fixation

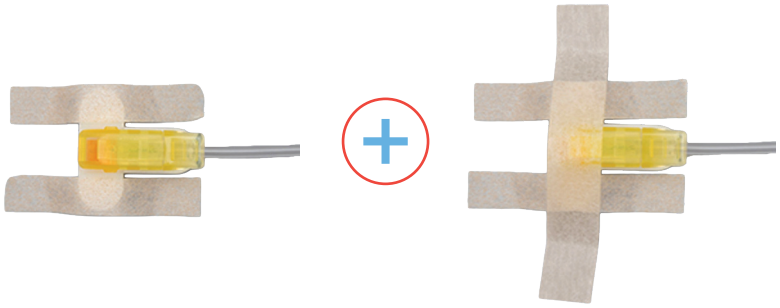

Tape down both wings, as shown.

OR



Tape across the wings or in an X-pattern, as shown.

2. Stabilize

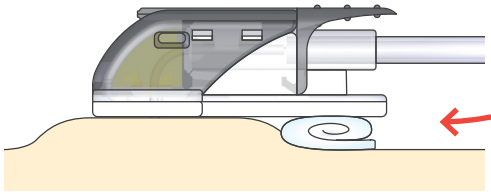

Placing gauze under the needle base helps stabilize the needle and minimize movement.



Avoid taping along the lower part of the needle housing. Doing so may unintentionally activate the safety mechanism.

3. U-Turn and Omega

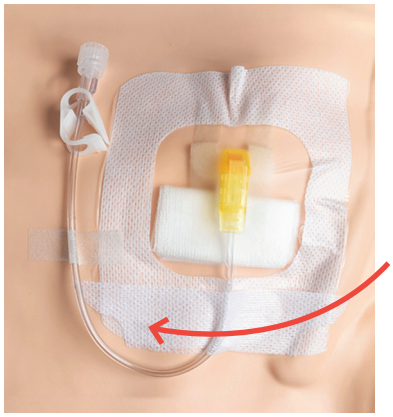

Forming a U-turn with the tubing and using the omega technique to secure it, as shown, helps prevent needle movement.



Omega technique





NIPRO Live Longer. Live Better.

NIPRO Corporation
3-26 Senriokashinmachi, Settsu-shi, Osaka 566-8510, JAPAN. | www.nipro.co.jp

NIPRO

SAFETOUCH™

Huber Infusion set



Reference pictures

Tape

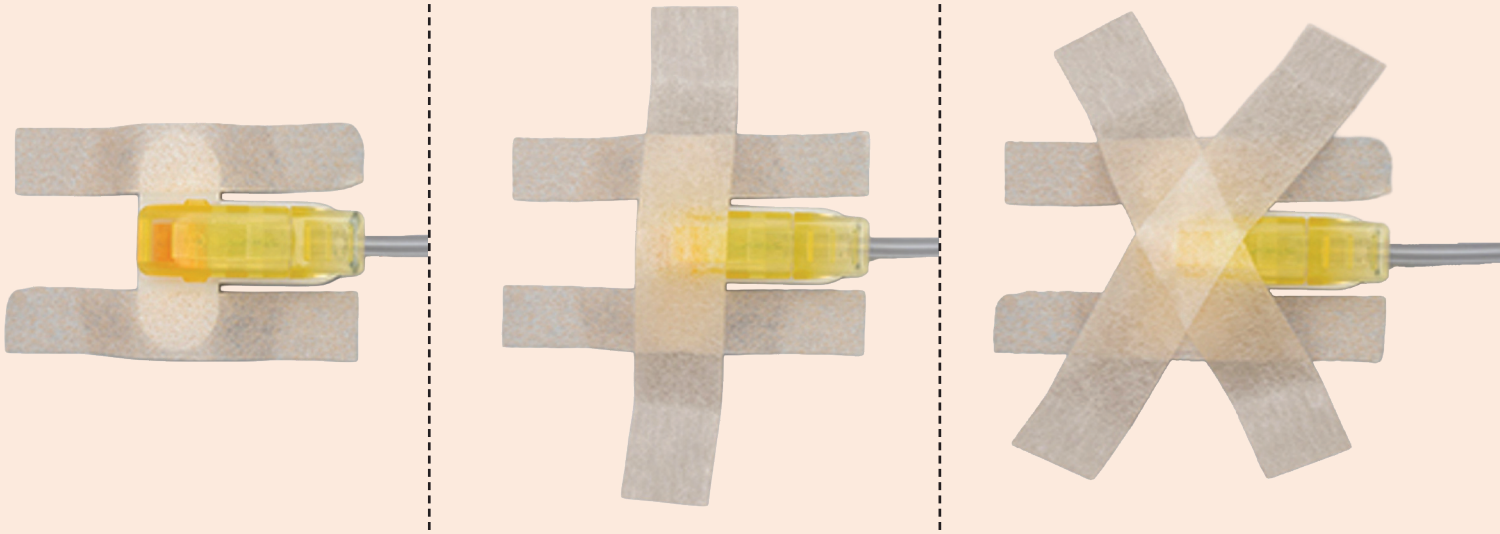

U Tubing



Omega technique

